

BEST AVAILABLE COPY

Fig. 1



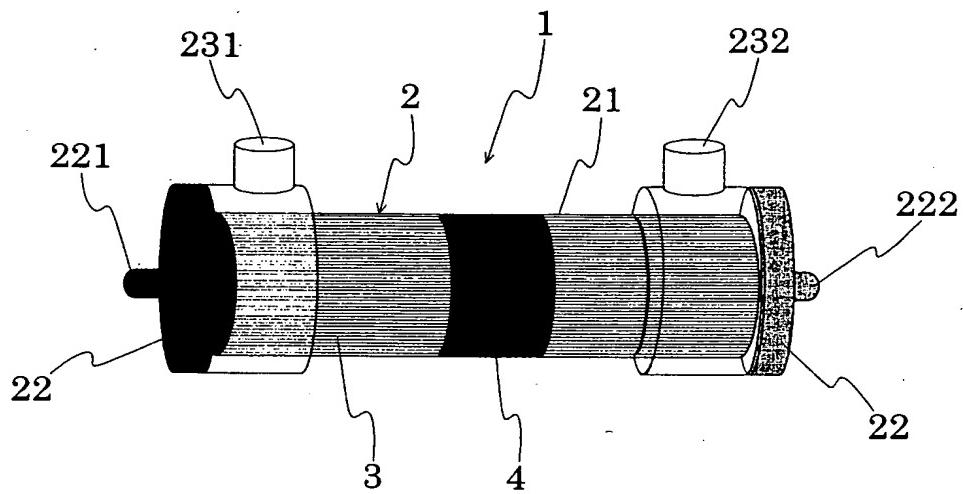


Fig. 2

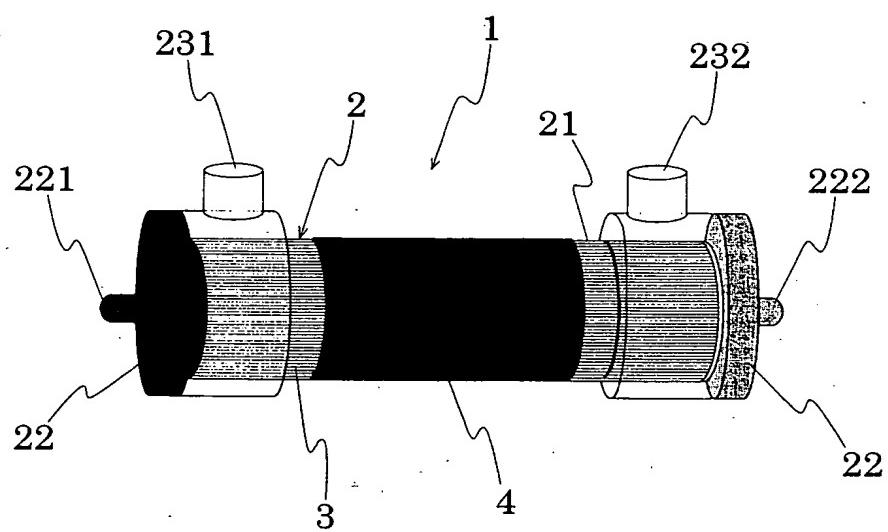


**Fig. 3**


**BEST AVAILABLE COPY**

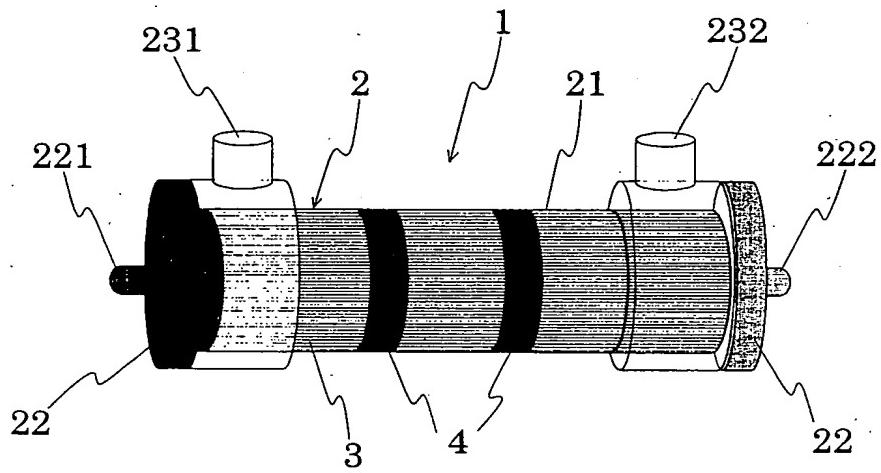


**Fig. 4 (a)**

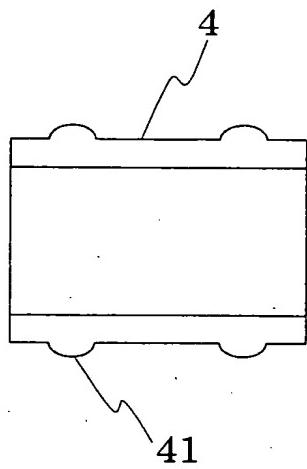

**Fig. 4 (b)**

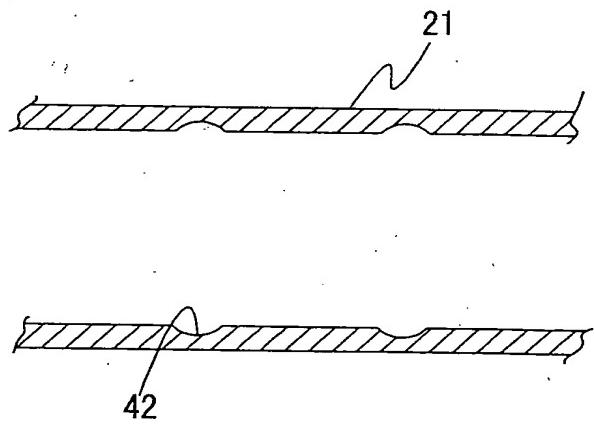


**Fig. 5**

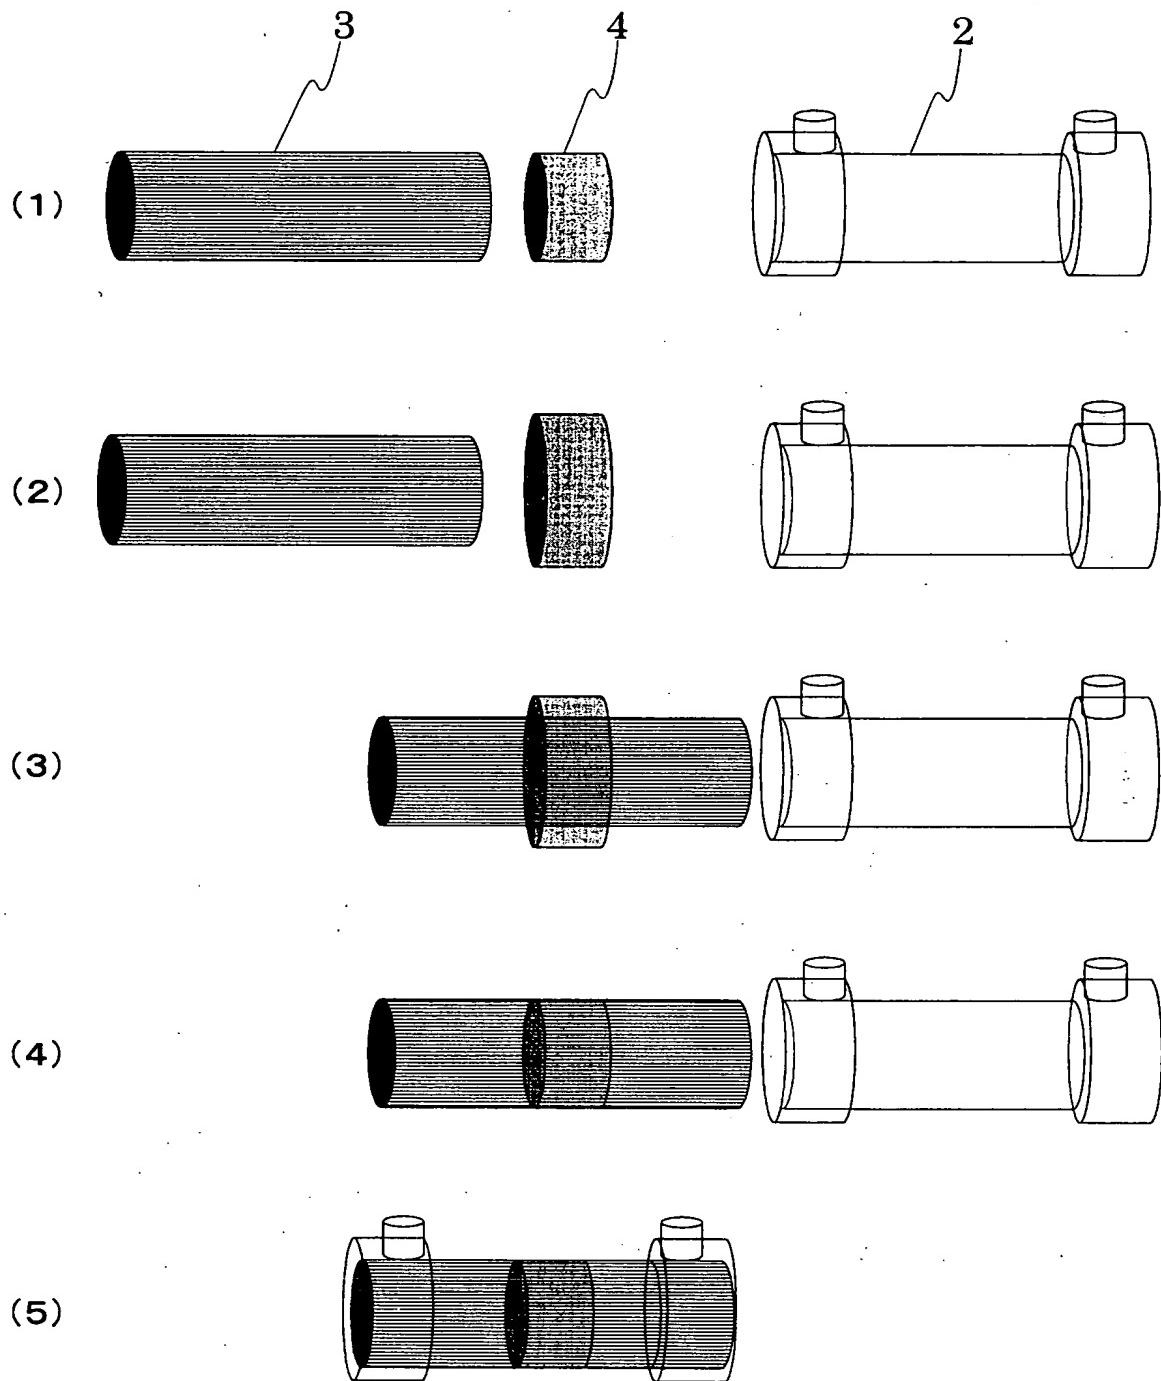


**Fig. 6**


PRESSURE DISTRIBUTION INSIDE DIALYZER

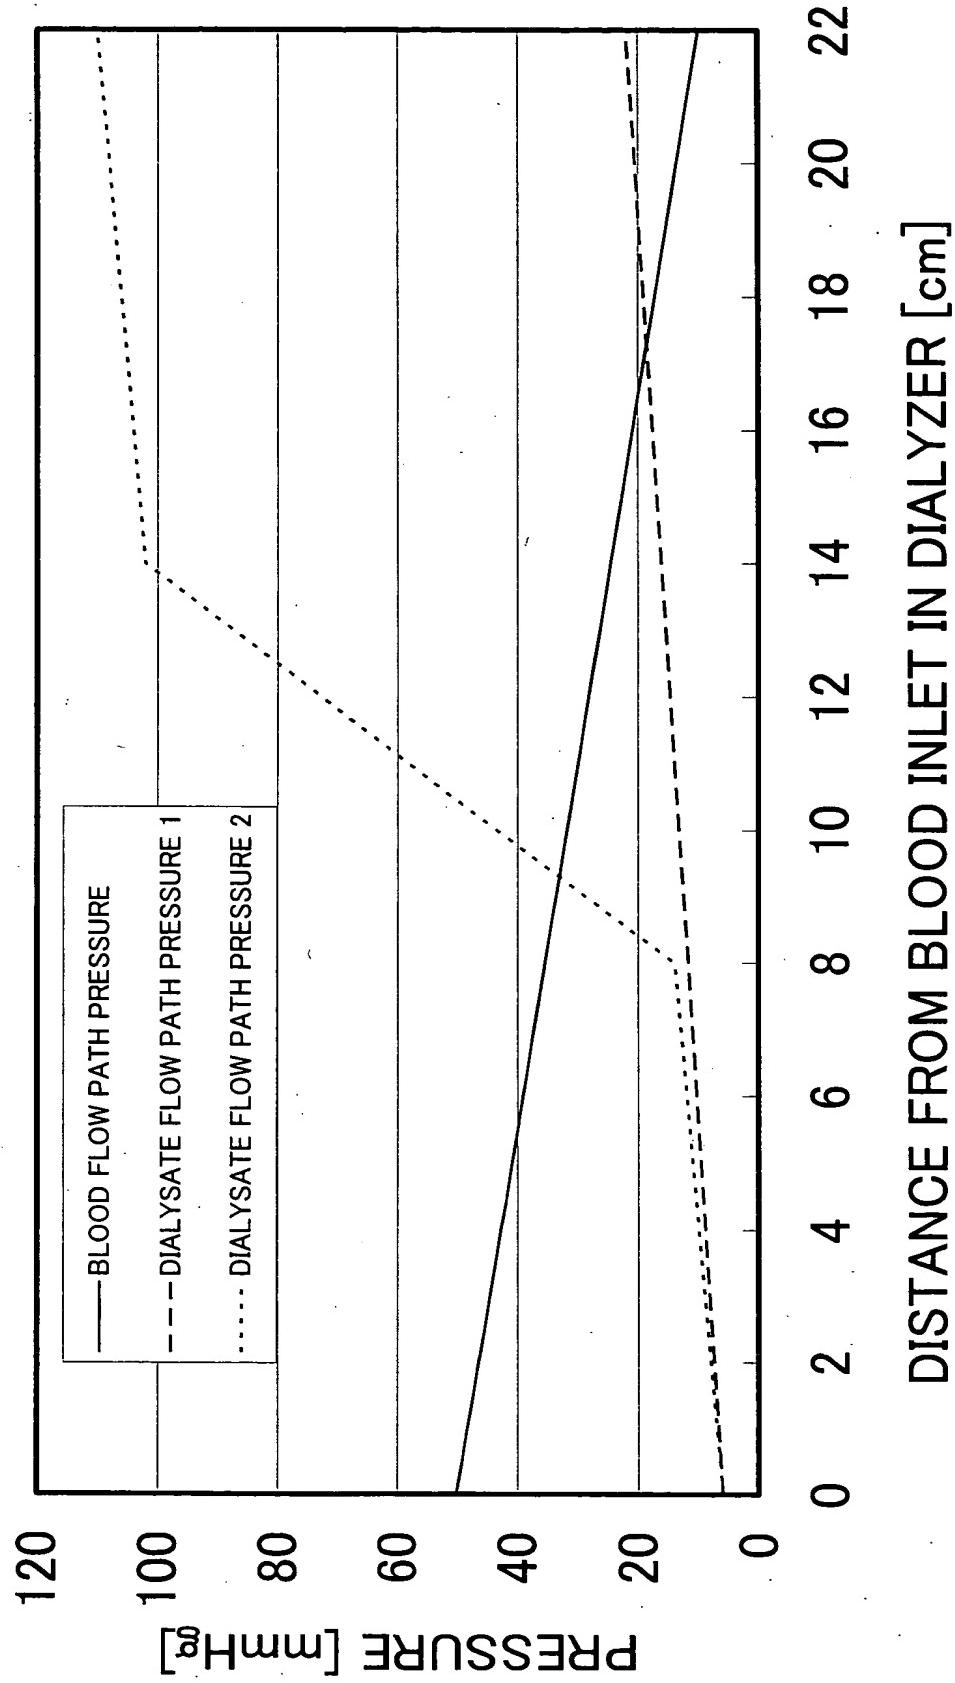


**Fig. 7**

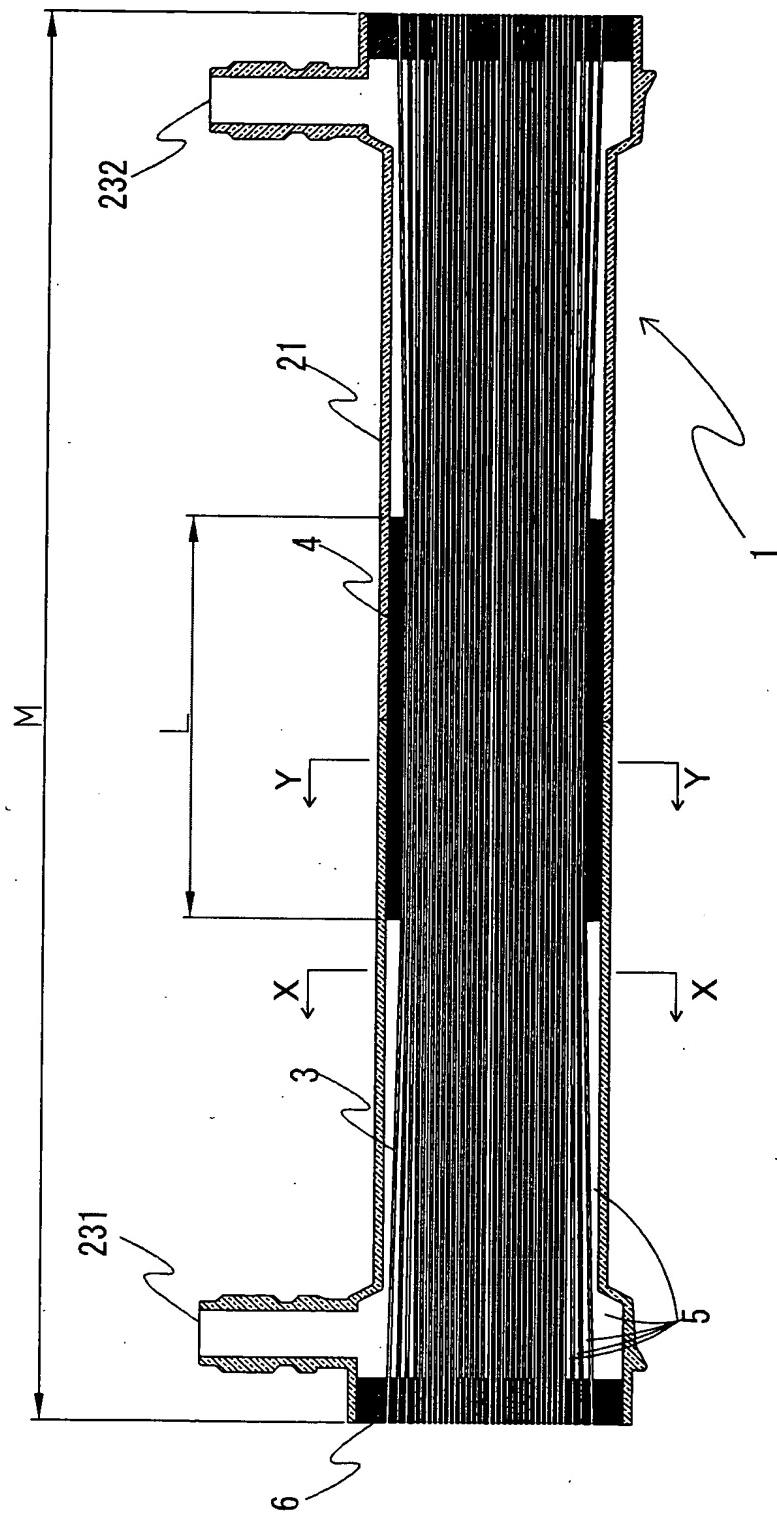

**Fig. 8**

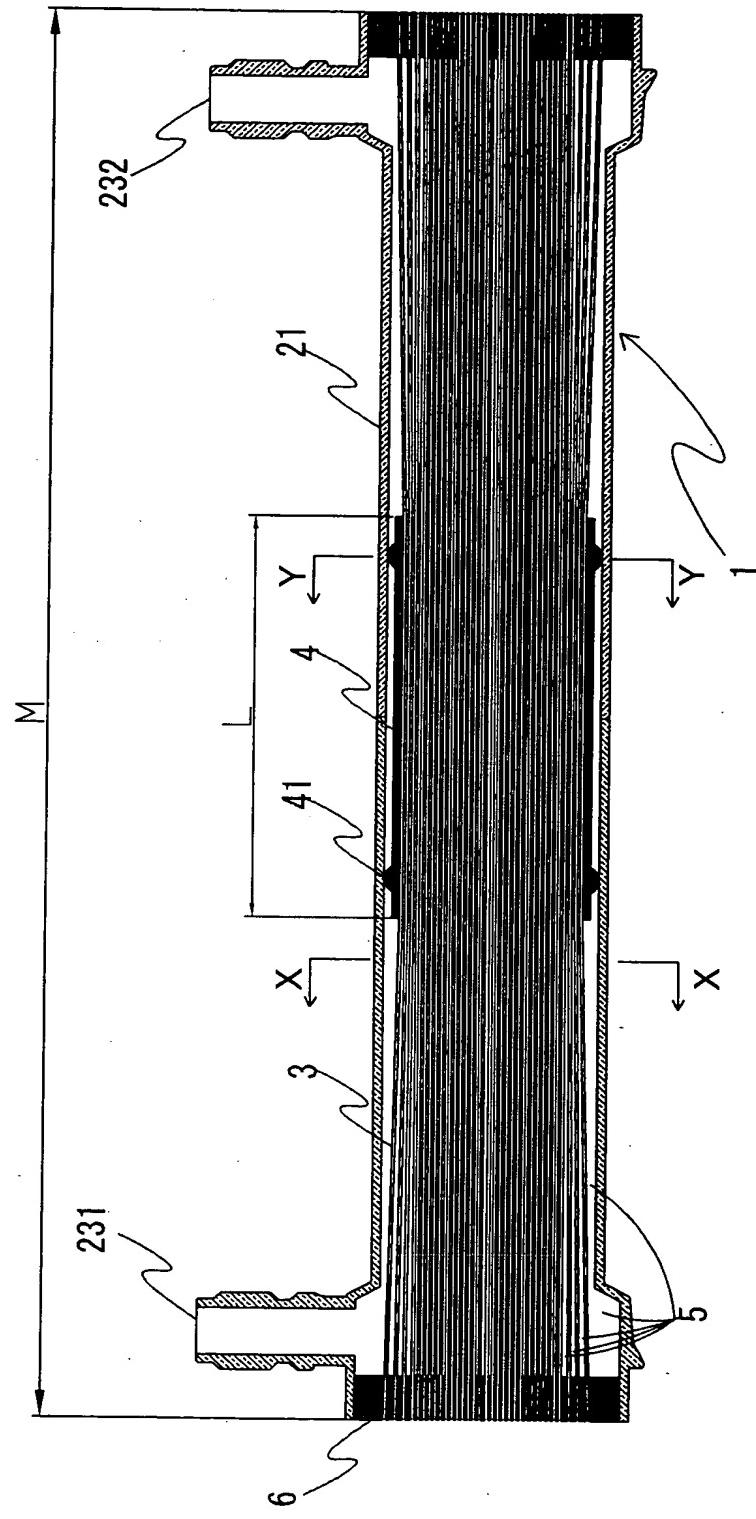


**Fig. 9**

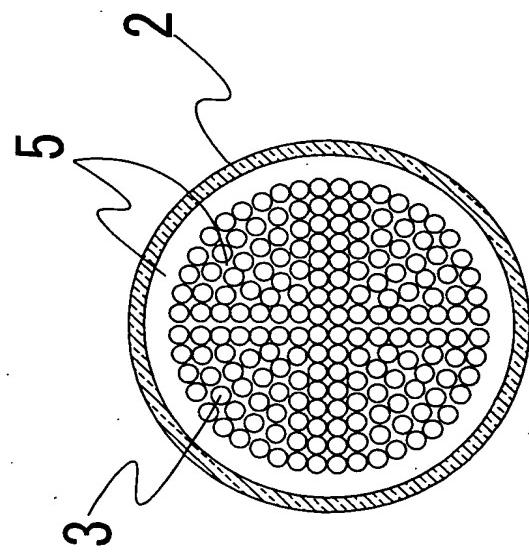

X-X

**Fig. 10**

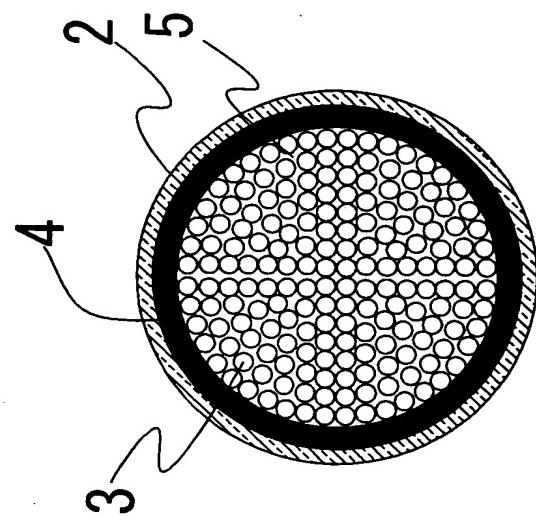

Y-Y